
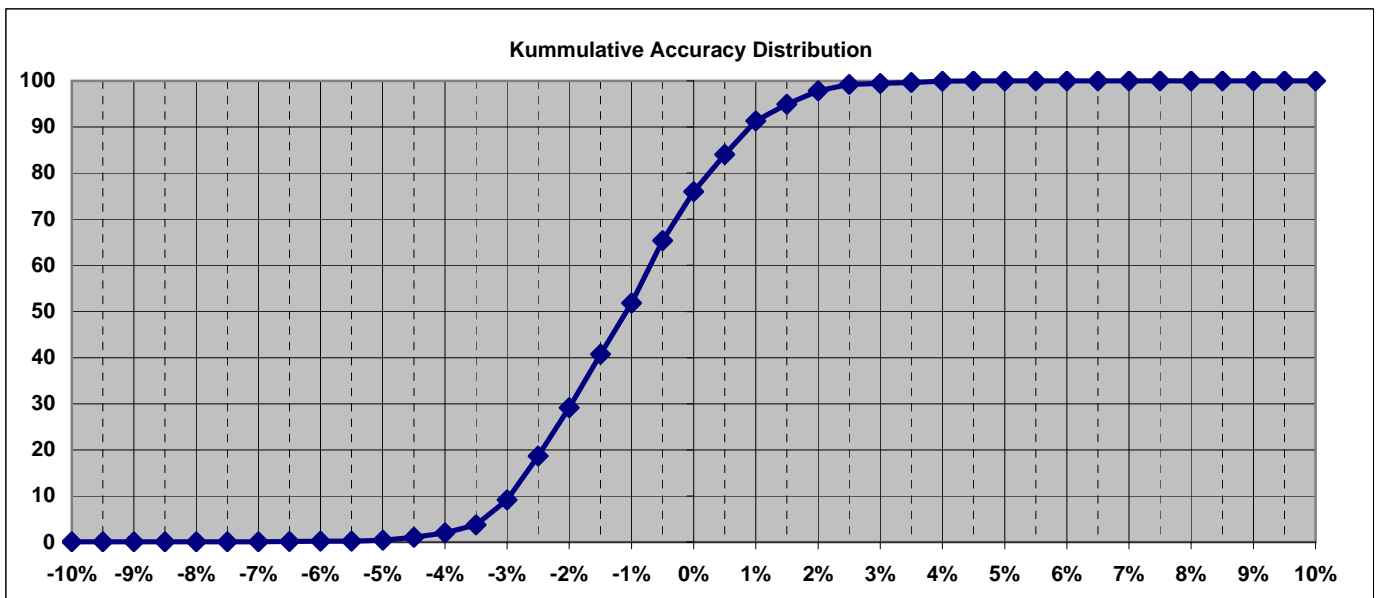


### Calibration Check of FACES EasyOne

110 EasyOne devices

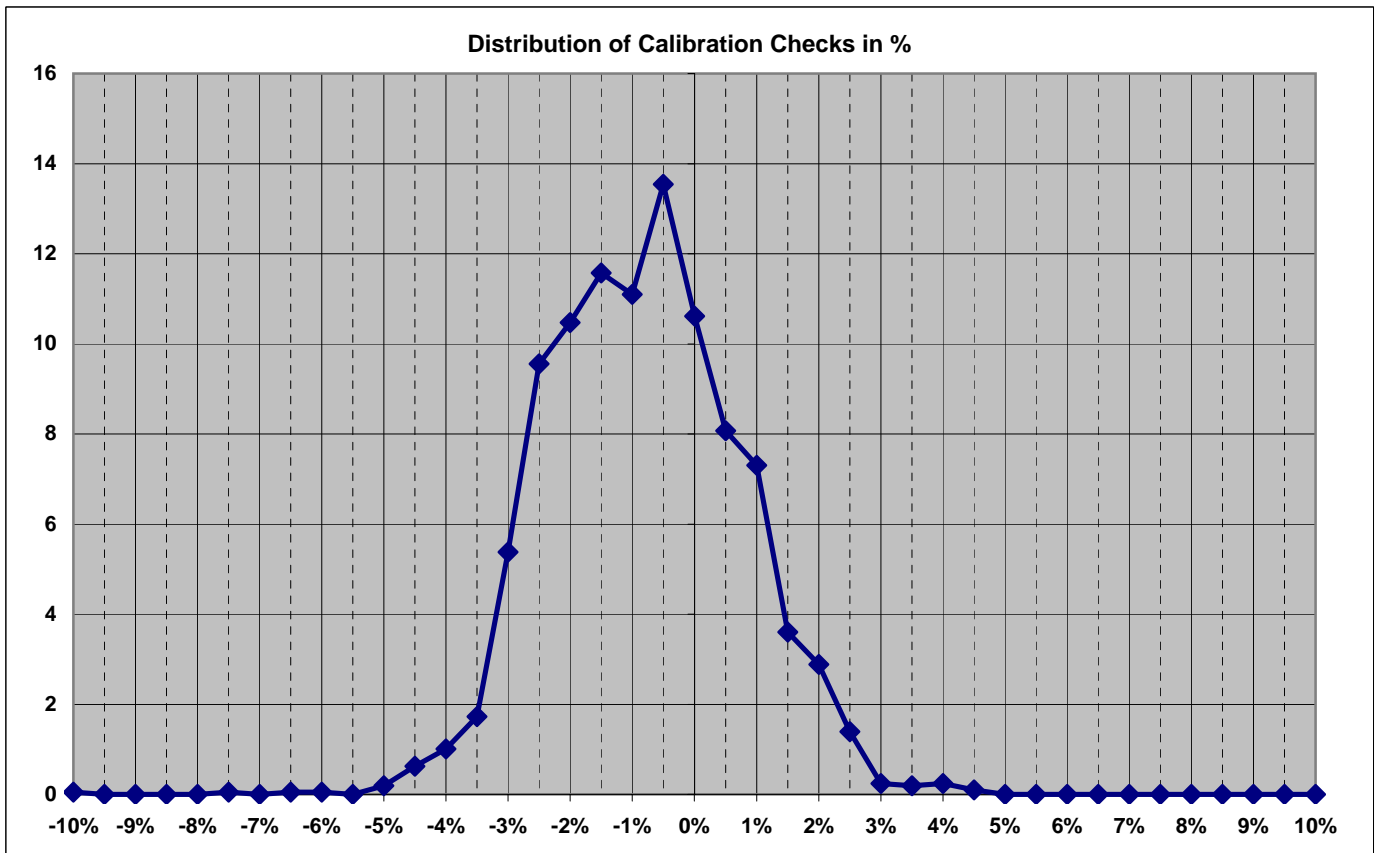

Accuracy Range	%
Within +/- 3.5%	97.6
Within +/-3%	95.7
Within +/- 2%	79.2
Within von +/-1%	50.6

Number of deleted trials outside +/-25%:  
 Number of calibration checks  
 Date range

71                      1.68%  
 4166  
 November 2000 to March 2004