
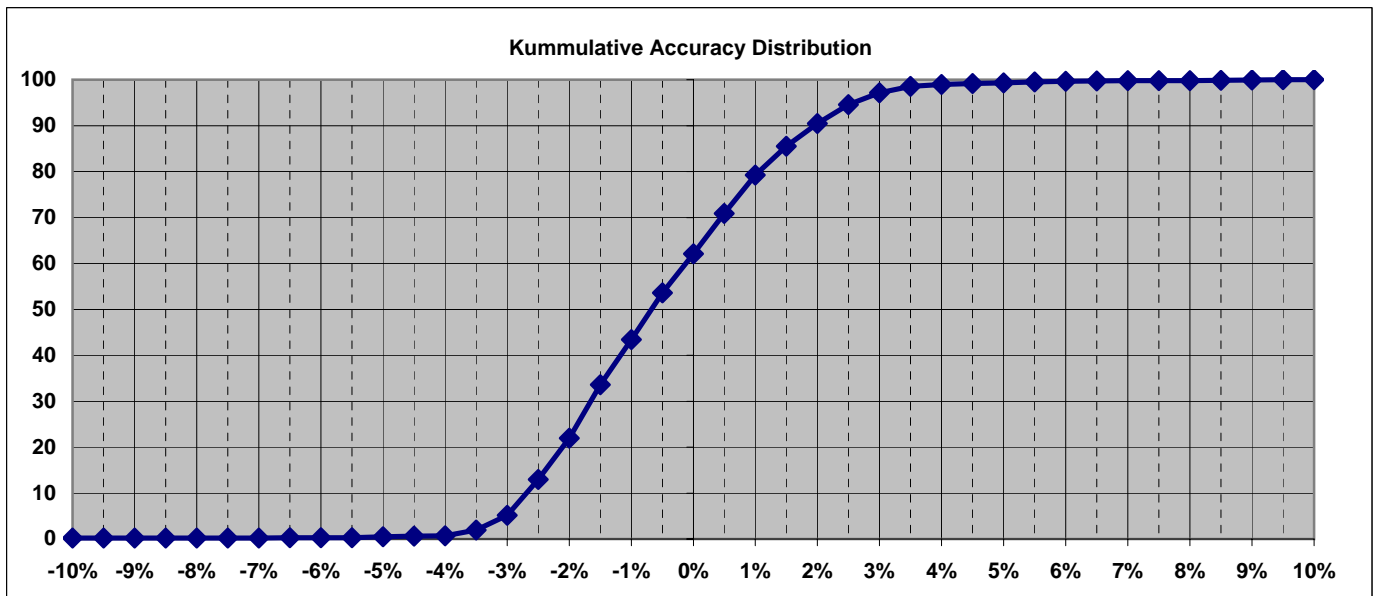


Calibration Check of World Trade Center EasyOne

13 EasyOne devices

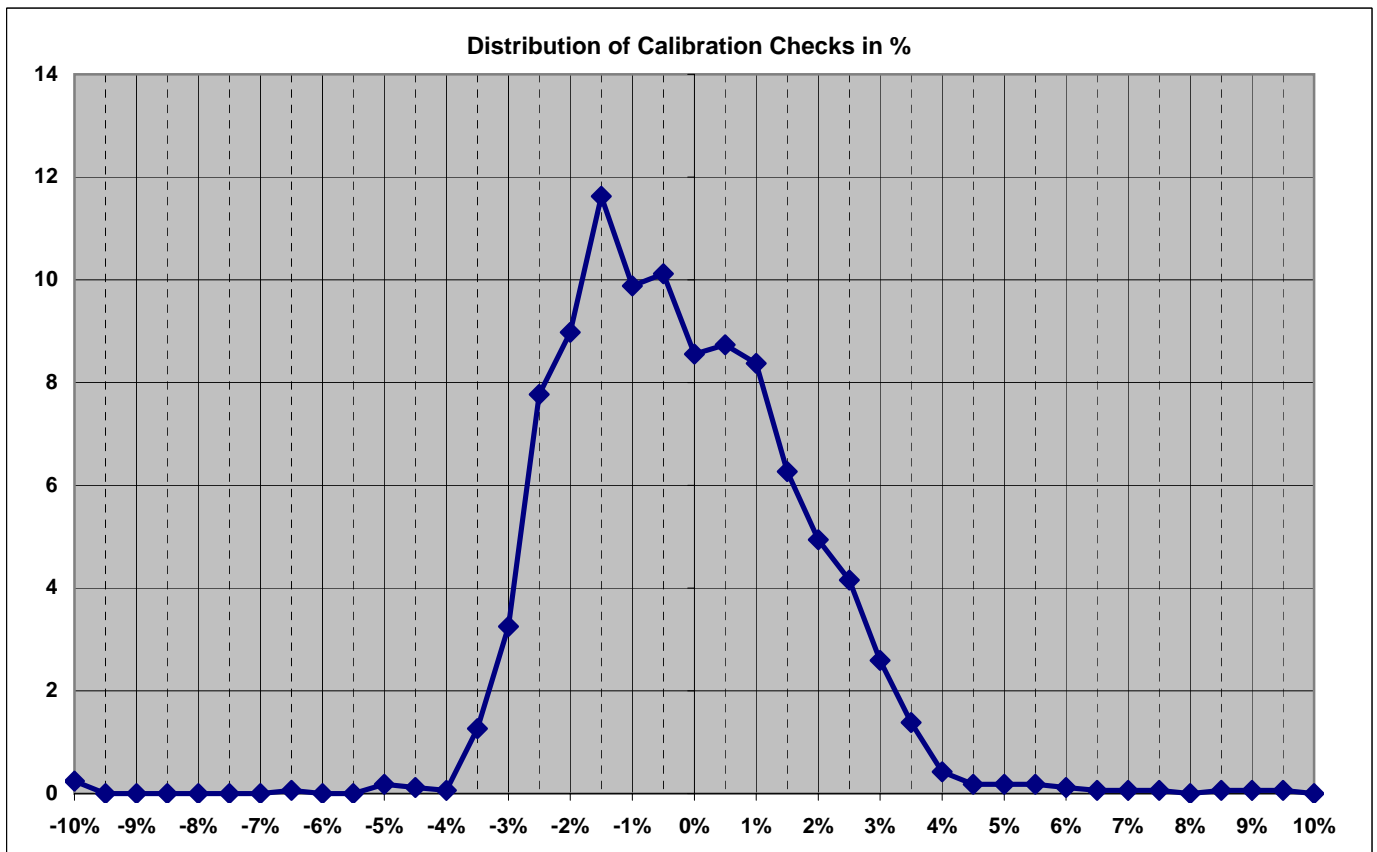

| Accuracy Range | % |
|------------------|------|
| Within +/- 3.5% | 97.9 |
| Within +/-3% | 95.2 |
| Within +/- 2% | 77.5 |
| Within von +/-1% | 45.7 |

Number of deleted trials outside +/-25%: 0
 Number of calibration checks 1667